


## Certificate of Calibration

Date Tested: 2011-03-28  
Model: Survey Meter SM 7 D  
Serial Number: SM7D110028  
Ambient Temperature T : 15,0 °C  
Ambient Air Pressure p : 963 hPa  
Calibration Source: Co-60 Photon energy 1.25 MeV  
Measuring value: count rate [cps]

Dose rate Co-60:

dose rate [ $\mu\text{Sv/h}$ ]	Reading count rate [cps]	response [cps / $\mu\text{Sv/h}$ ]
100	650,0	6,5

Energy Response Survey Meter SM7D (typical values):

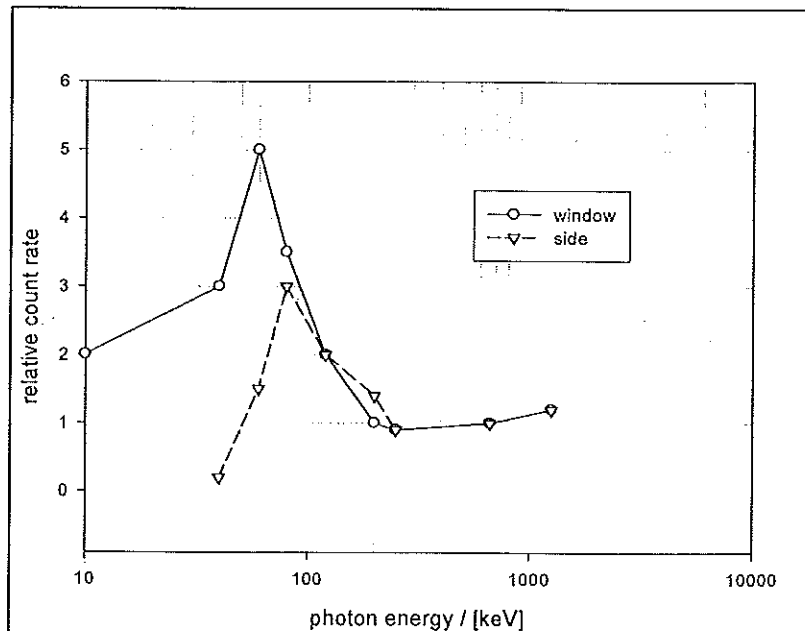

Tested by :

  
Steve Bahn