


Certificate of Calibration

Date Tested: 2011-04-04
Model: Survey Meter SM 3 D
Serial Number: SM3D110012
Ambient Temperature T : 16,0 °C
Ambient Air Pressure p : 968,0 hPa
Calibration Source: Cs-137 Photon energy 0.662 MeV
Measuring value: Ambient equivalent dose rate $\mu\text{Sv/h}$

Dose rate Cs-137

dose rate [$\mu\text{Sv/h}$]	Reading [$\mu\text{Sv/h}$]	deviation [%]
160	155,0	-3,13

Energy Response counting tube:

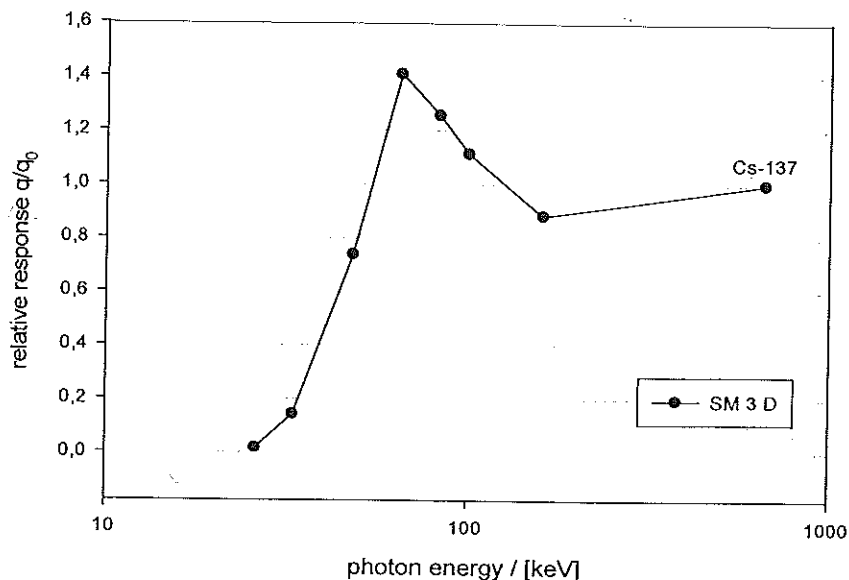

Tested by :

Jens Bieber
Jens Bieber